
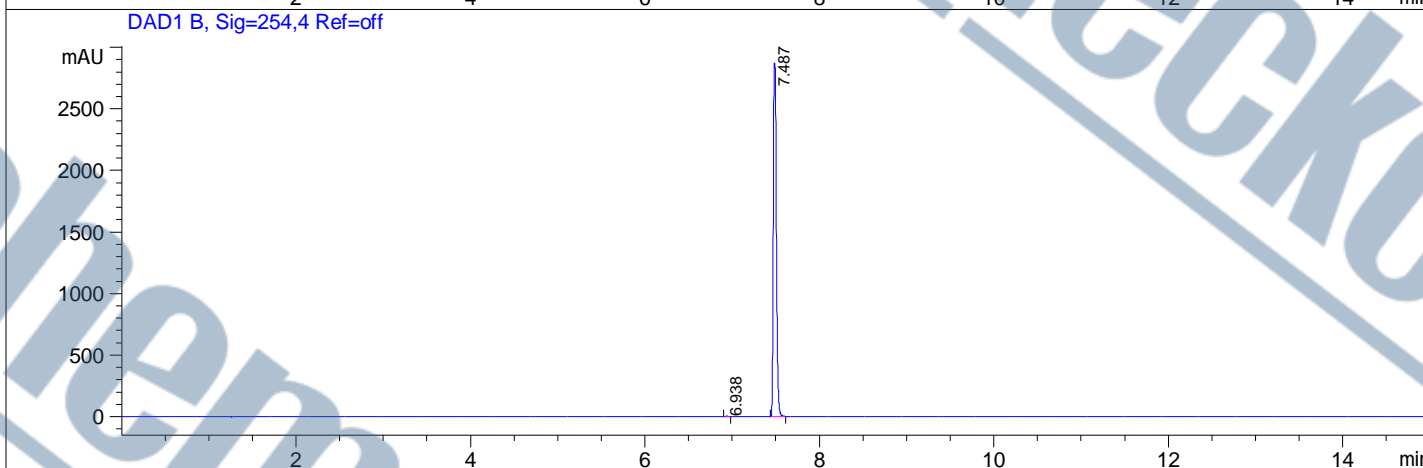


File D:\DATA\T114\CP-000B177-00323-HPLCA004.D
 Injection Date : 30-May-11, 15:28:12 Tgt Mass(EZX) :
 Sample Name : CP-000B177 Location : P1-E-06
 Acq. Operator : HPLCA004 Inj : 0
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M
 Analysis Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M
 Sample Info :
 Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
 Gradient: 0min 5%B,3min 5%B,10min 95%B,15min 95%B
 Flow Rate: 1.2 ml/min
 Column: Eclipse XDB-C18,4.6*150mm,5um
 Oven Temperature: 40 C

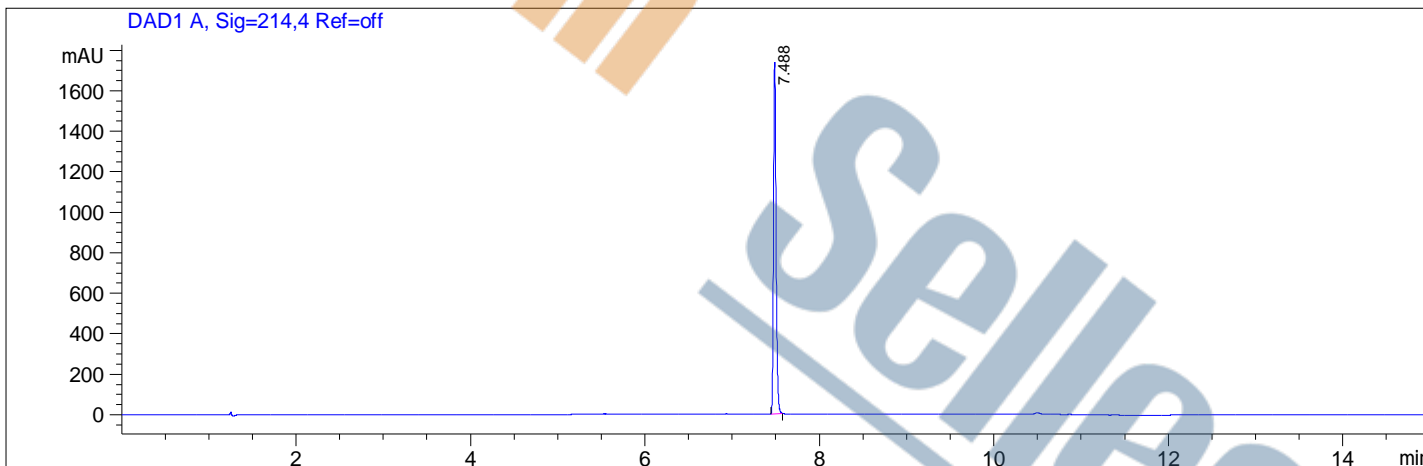

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
7.49	0.03	3566.66	1738.99	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
6.94	0.03	10.88	5.17	0.15
7.49	0.04	7058.52	2870.03	99.85